




An ISO 9001 & 14001 Co.

MEDICAL & HOSPITAL EQUIPMENT

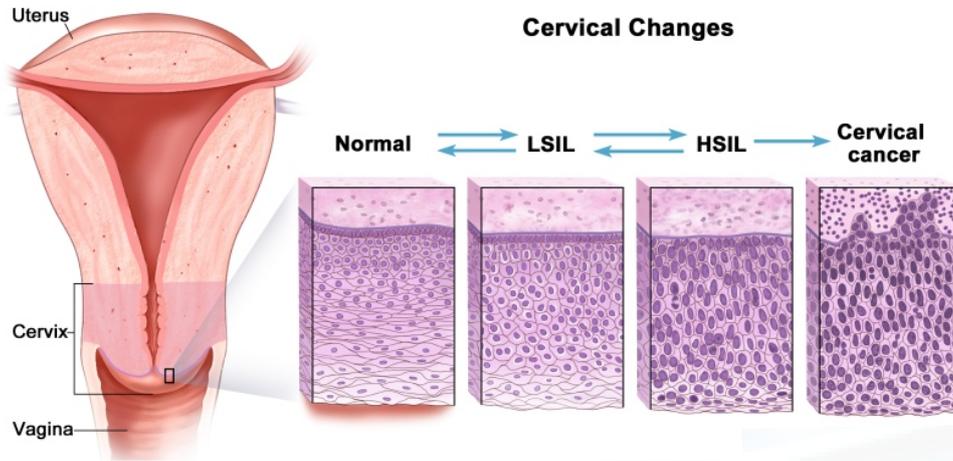

MODEL NO.:- RAJAS-CT5-13

(Anatomical model for cervical lesion screening)

Specification:-

Anatomical model for cervical lesion screening

This poseable cervical model is an excellent patient education tool for practitioners and healthcare staff.

Using this brain model

Allows the following pathologies to be studied:

Erosion of the cervix

Linear laceration collar

Cervix with polyp

Cervix with inflamed nabothian cyst

Cervix affected by carcinoma, Mounted on transparent plexiglass support, Instructions for use included, To be delivered complete to the site of use

Delivery will be made to the following sites 2 at the DSF in Ouagadougou and 4 by DRS DRS center-south (Manga) DRS plateau-central (Ziniaré), DRS Center-north (KAYA), DRS EST (Fada) DRS CASCADES (Banfora) DRS north Ouahigouya, DRS CENTRE-EST (Tenkodogo), DRS Boucle du Mouhoun (Dédougou) DRS Center Ouagadougou, DRS Hauts-Bassins (Bobo) DRS Sahel (DORI) South-west (Gaoua)

RAJAS ENTERPRISES (INDIA)

#59, Phase-1, Sector-1, HSIIDC, Industrial Estate, SAHA, Ambala Cantt-133104 (India)

Email: rajasmedical@gmail.com, rajasglass@gmail.com

www.rajasenterprises.com